

Pin Assignment

Connector	Pin	Signal	Remarks
①	1	Ethernet TxD+	-
	2	Ethernet RxD+	-
	3	Ethernet TxD-	-
	4	Ethernet RxD-	-

Pin assignment of Ethernet interface

Connector	Pin	Function	Remarks
②	1	+24 VDC ¹	Power supply for interface module and sensors
	2	+24 VDC ¹	
	3	GND	
	4	GND	
	5	Shield	

Pin assignment of power connection

1) Permissible supply voltage range 11 - 30 V

You can download a PDF of the detailed operating instructions from our website:


www.micro-epsilon.de/download/manuals/man--IF2008-ETH--en.pdf

MICRO-EPSILON MESSTECHNIK GmbH & Co. KG
Koenigbacher Str.15
94496 Ortenburg / Germany
Tel. +49 8542 / 168-0 / Fax +49 8542 / 168-90
e-mail info@micro-epsilon.com
www.micro-epsilon.com

X9771379-A012090HDR



Connector	Pin	Function	Remarks
③	1	External entrance 1	-
	2	External entrance 2	-
	3	External entrance 3	-
	4	External entrance 4	-
	5	External output 1	-
	6	External output 2	-
	7	External output 3	-
	8	External output 4	-
	9	n.c.	-
	10	n.c.	-
	11	Voltage output	LLL = +5 V, HLL = +24 V
	12	GND	-



Pin assignment I/O interface

Connector	Pin	Signal IF2008 ETH	Signal Encoder
④a	1	A+	A+
	2	A-	A-
④b	3	B+	B+
	4	B-	B-
④c	5	R+	R+
	6	R-	R-
④d	7	+24 VDC ¹	n.c.
	8	Laser ON- ¹	n.c.
④e	9	Multi-function output ¹	n.c.
	10	ERROR input ¹	n.c.
④f	11	+5 VDC	+5 VDC
	12	GND	GND

Pin assignment encoder interface

1) Only for sensors

Connector	Pin	Signal IF2008 ETH	Signal ILD 1420	Signal ILD 2300	Signal IFC 24xx
④	1	TRG+	n.c.	TRG+	n.c.
	2	TRG-	n.c.	TRG-	n.c.
	3	TxD+	RxD+	RxD+	TxD+
	4	TxD-	RxD-	RxD-	TxD-
	5	RxD+	TxD+	TxD+	RxD+
	6	RxD-	TxD-	TxD-	RxD-
	7	+24 VDC	+U _B	+U _B and Laser ON+	n.c.
	8	Laser ON-	Laser ON-	Laser ON-	n.c.
	9	Multifunction output	Multifunction input	n.c.	TRG+ (HLL) ¹
	10	ERROR input	ERROR output	n.c.	n.c.
	11	+ VDC (only for encoder)	n.c.	n.c.	n.c.
	12	GND	GND	GND	GND

Pin assignment for sensor interface

1) Bridge for HLL level is set on the IFC 24xx controller.



Assembly Instructions
IF2008/ETH



Intended Use

The IF2008 ETH interface module is designed for use in industrial and laboratory applications. It is used to convert the MICRO-EPSILON internal sensor protocol (RS422) to Ethernet.

The IF2008 ETH interface module must only be operated within the limits specified in the technical data. The IF2008 ETH interface module must be used in such a way that no persons are endangered or machines and other material goods are damaged in the event of malfunction or total failure of the IF2008 ETH interface module. Take additional precautions for safety and damage prevention in case of safety-related applications.

Warnings

Connect the power supply and the display/output device according to the safety regulations for electrical equipment.

> Risk of injury, damage to or destruction of the interface module

The supply voltage must not exceed the specified limits.

> Risk of injury, damage to or destruction of the interface module

Avoid shocks and impacts to the interface module.

> Damage to or destruction of the interface module

Notes on CE Marking

The following apply to the IF2008 ETH interface module:

- EU Directive 2014/30/EU
- EU Directive 2011/65/EU, "RoHS"

Products which carry the CE mark satisfy the requirements of the EU directives cited and the relevant applicable harmonized European standards (EN). The measuring system is designed for use in industrial environments and laboratory applications.

The EU Declaration of Conformity is available to the responsible authorities according to EU Directive, article 10.




Proper Environment

Protection class: IP65 (When all plugs are connected.)

- Temperature range:
 - Operation: 0 ... +50 °C (+32 ... +122 °F)
 - Storage: +5 ... +50 °C (+41 ... +122 °F)
- Humidity: 5 - 95 % (non-condensing)
- Ambient pressure: Atmospheric pressure

Installation and Assembly

Ensure careful handling during installation and operation.

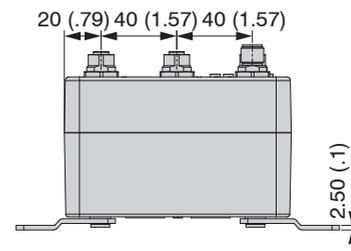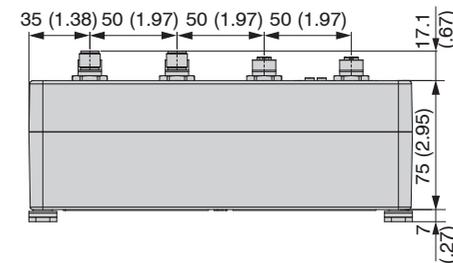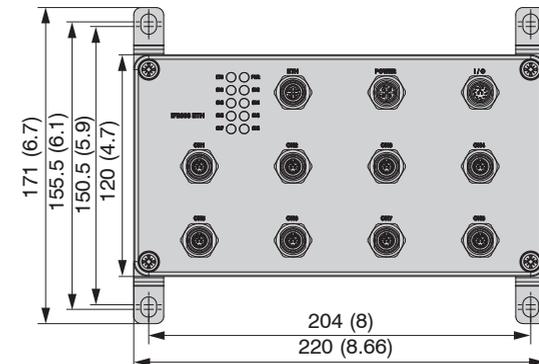


Dimensional drawings
IF2008 ETH interface
module, dimensions in mm
(inches), not to scale

Pin Assignment


LEDs

LED	LED color	Description
①	Off	Power supply off
	Green	Interface module is ready for operation
	Orange	Interface module is in bootloader/flash mode
	Red	Initialization of the interface module
②	Off	No Ethernet connection
	Orange	Connection between PC and interface module (100 Mbps)
	Flashing	Data transmission between PC and interface module
③	Off	No sensor/encoder selected
	Green	Interface set for sensor
	Orange	Interface set for sensor



Description of status LEDs IF2008 ETH interface module

Connector Overview

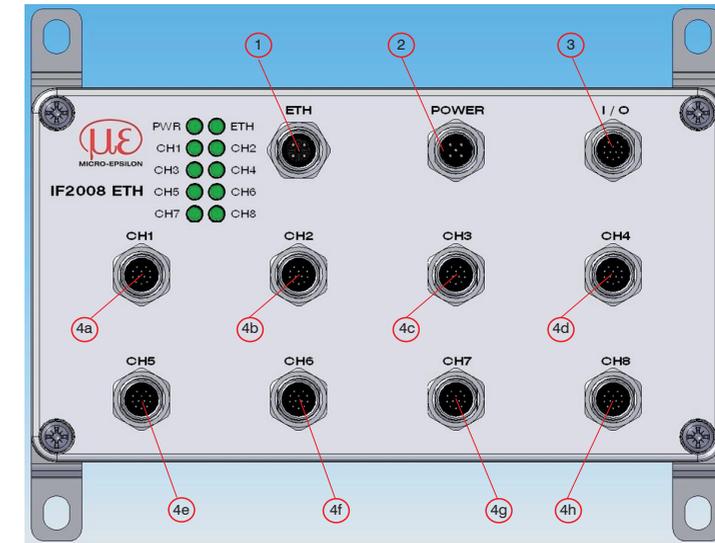

Plug-in connections IF2008 ETH interface modul

Connector	Description
ETH	Flange socket, 4-pin, type Binder 09 3732 500 04 for Ethernet connection
POWER	Flange connector, 5-pin, type Binder 09 3441 600 05 for power connection
I/O	Flange connector, 12-pin, type Binder 09 3491 600 12 for power connection
CH1 - CH8	Flange socket, 12-pin, type Binder 09 3492 600 12 for sensor/encoder connection

Overview of plug-in connections